

USING THE PLATE HOLDER ON THE FACSMELODY


UNC FLOW CYTOMETRY CORE FACILITY

EJECT PLATE HOLDER


1. Insert ACDU into Sort block



2. Navigate to “2 Set Up Sort” > Select Plate and define sorting parameters

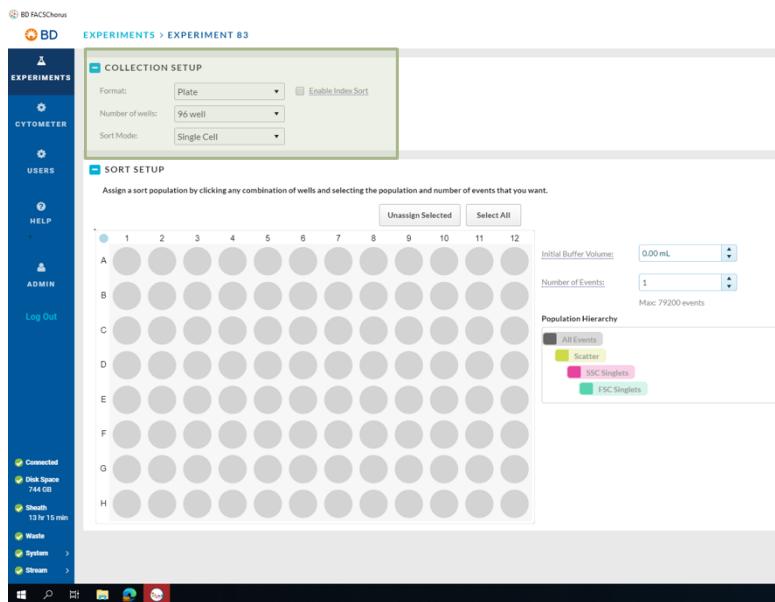

3. Navigate to “3 Sort” >Select EJECT in the Sort Status Menu

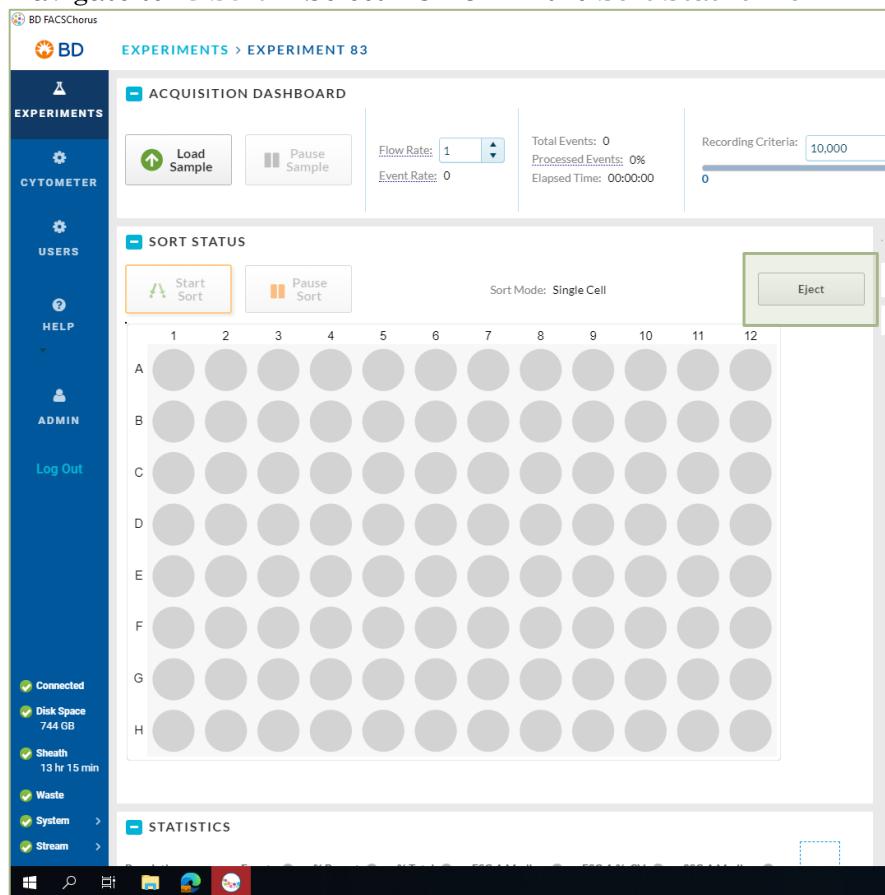


4. Place Plate on Plate holder and proceed to sort

RETRACT PLATE HOLDER

1. Keep ACDU in Sort Block



2. Navigate to the “2 Set up Sort” > Select TUBES

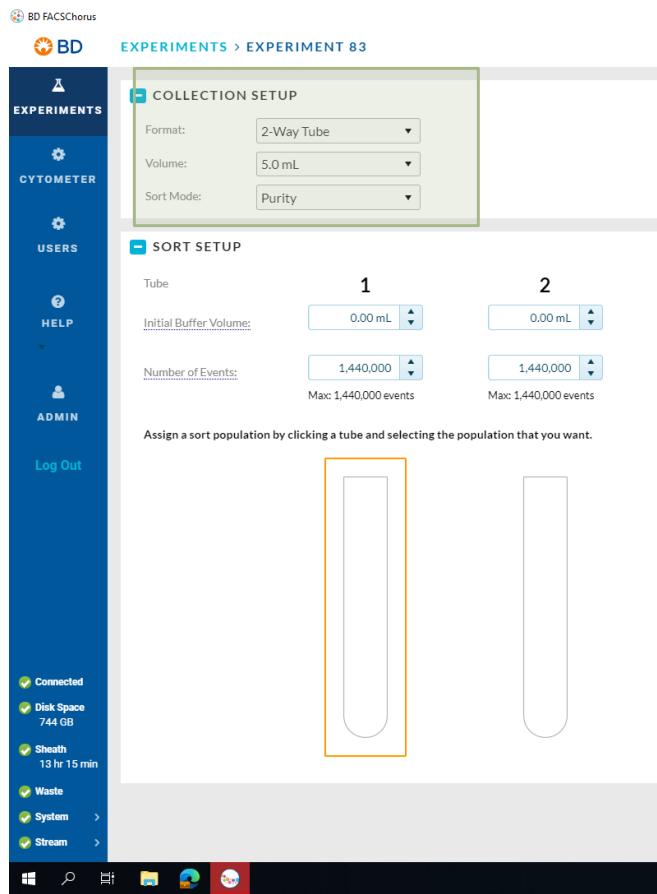

3. Navigate to “3 SORT” > Select RETRACT in Sort Status Menu

