


GI procedures device (PM or ICD) management protocol summary

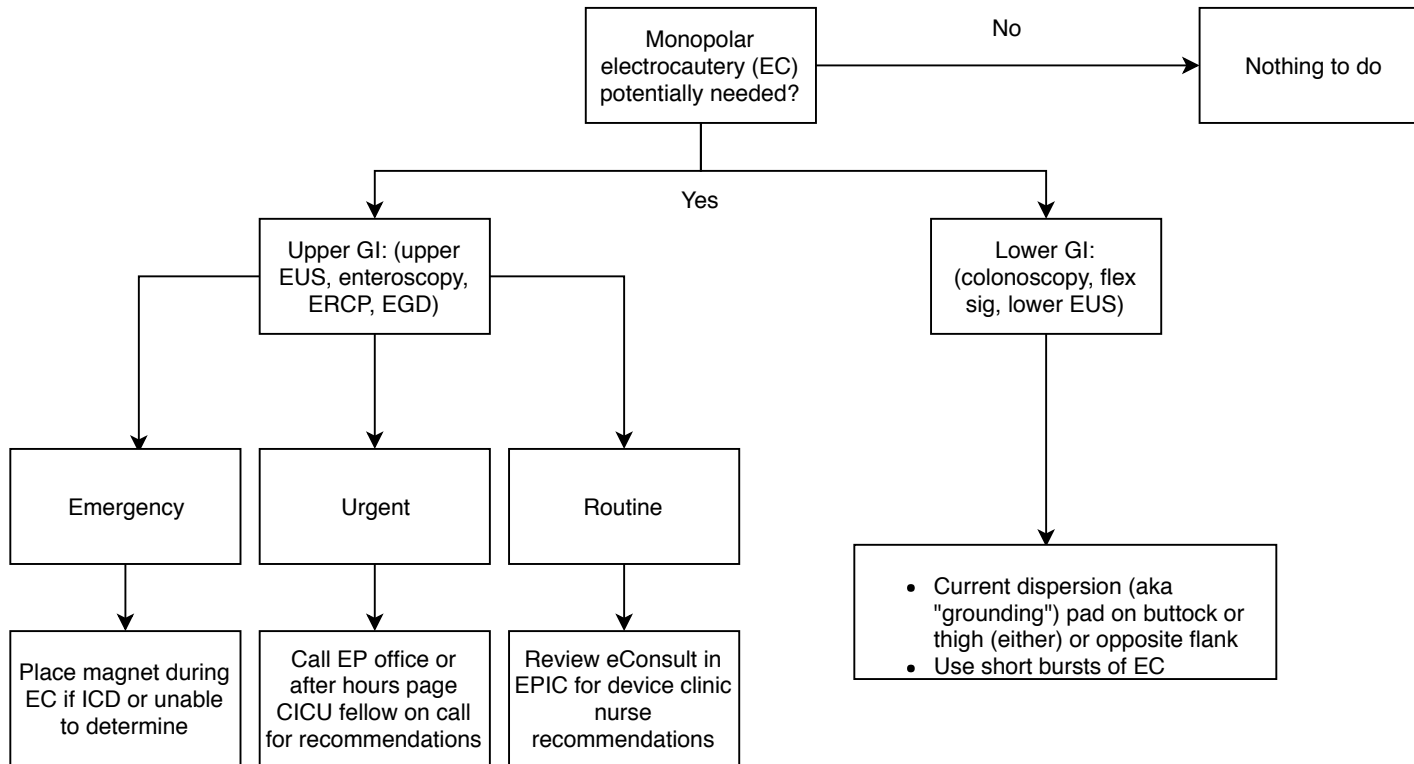

EP office:

984-974-5121

General Recommendations

- During monopolar EC, place and secure magnet over device when recommended and remove when EC is complete
- If pacing noted on EKG rhythm strip - monitor for inhibition (low heart rate) during EC
- Use short bursts of EC
- Not necessary to check device post procedure

